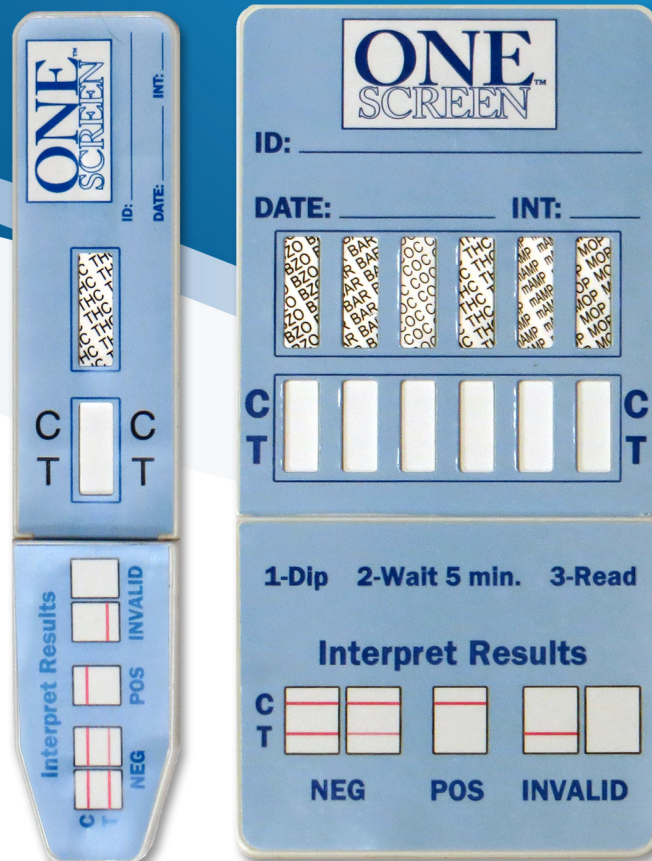# Corporate Drug Testing Made Simple!

OneScreen™

One Step Dip Card

The OneScreen Dip Card is our top quality Urine Dip Card. Fast, accurate, and affordable. Your search is over.

- ▶ **Simple dip and read procedure**
- ▶ **Room temperature storage**
- ▶ **Laboratory accurate**
- ▶ **Detects 1-12 drugs**
- ▶ **Results in minutes**
- ▶ **24-Month Shelf Life**
- ▶ **99.9% Accuracy**
- ▶ **Customizable, choose from 27 drugs**

BUP CLIA WAIVED PPX
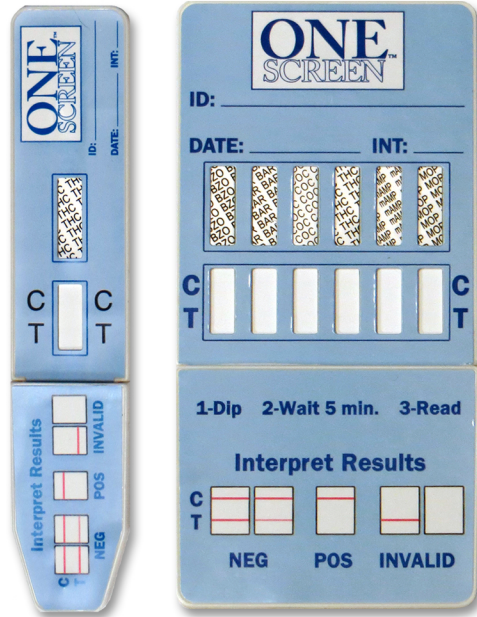
ASC American Screening Corporation

Ron Kilgarlin
318.798.3306 ext. 11
ron@americanscreeningcorp.com

PH: 318.798.3306
FX: 318.798.3386
TF: 1.866.526.2873

OneScreen™
Dip Card

Corporate Drug Testing Made Simple

Detects the presence of drugs in minutes.
It's drug testing efficiency you can count on.

1-Dip 2-Wait 5 min. 3-Read

Interpret Results

NEG   POS   INVALID

+FDA Cleared *CLIA Waived		
+Amphetamine	AMP300	300ng/ml
+*Amphetamine	AMP	1000ng/ml
+*Barbiturates	BAR	300ng/ml
+*Benzodiazepines	BZO	300ng/ml
+*Buprenorphine	BUP	10ng/ml
+Cocaine	COC150	150ng/ml
+*Cocaine	COC	300ng/ml
+*Ecstacy	MDMA	500ng/ml
Marijuana	THC20	20ng/ml
+*Marijuana	THC	50ng/ml
+*Methadone	MTD	300ng/ml
+Methamphetamine	mAMP500/MET500	500ng/ml
+*Methamphetamine	mAMP/MET	1000ng/ml
+*Opiates	OPI300/MOP	300ng/ml
+*Opiates	OPI	2000ng/ml
+*Oxycodone	OXY	100ng/ml
+*Phencyclidine	PCP	25ng/ml
+*Propoxyphene	PPX	300ng/ml
+*Tricyclic Antidepressants	TCA	1000ng/ml
Specialty Drugs		
Alcohol	ALC	20mg/dl
EDDP	EDDP100	100ng/ml
EDDP	EDDP	300ng/ml
Fentanyl	FEN	100ng/ml
K2/Spice	K2	50ng/ml
Ketamine	KET	1000ng/ml
Methaqualone	MQL	300ng/ml
Methylphenidate	MTHP	300ng/ml
Nicotine	COT	200mg/ml
Tramadol	TRA	300ng/ml

Pull

DO NOT ALLOW URINE
TO TOUCH PLASTIC DEVICE

DO NOT ALLOW URINE
TO TOUCH PLASTIC DEVICE

URINE

Adulterant Chart

TEST	ABNORMAL (LOW)	NORMAL	ABNORMAL (HIGH)
Oxidant/ PCC		Negative	
S. G.	1.000	1.003 1.005 1.015 1.025	≥1.035
PH	2.0 3.0	4.0 7.0 9.0	10.0 11.0 12.0
NIT		0mg/dl 20mg/dl	50mg/dl 100mg/dl
GLUT			
CRE	0mg/dl	20mg/dl 100mg/dl	

① Remove OneScreen™ test from foil pouch at room temperature. Take off the cap revealing the testing strips.

② Immerse test vertically in the urine sample for at least 10-15 seconds. Do not allow the specimen to touch the device housing.

5min

③ Read at five(5)minutes. Results stable up to one (1)hours.

Interpretation of Results:

Negative
(2 Lines-Any indication of a line in both test and control fields is to be interpreted as a NEGATIVE)

Positive
(1 Lines)

Invalid
(No line(s) or no control line(s))